

MR-1, MR-12

Rocker-shakers



If you have any feedback on our products or services, we would like to hear from you.
Please send all feedback to:

Manufacturer:

SIA Biosan
Ratsupites 7 k-2, Riga, LV-1067, Latvia

Phone: +371 674 261 37



<https://biosan.lv>

Marketing e-mail: sales@biosan.lv

Support e-mail: support@biosan.lv

Contents

1. About this edition of instructions for use	3
2. Safety precautions	3
3. General information	4
4. Getting started	5
5. Operation – model MR-1	6
6. Operation – model MR-12	7
7. Specifications	8
8. Ordering information	9
9. Care and maintenance	9
10. Storage and transportation	10
11. Warranty	10
12. EU Declaration of conformity	11

1. About this edition of instructions for use

1.1. The current edition of the instructions for use (IFU) applies to the following models:

Model and name	Version
MR-1, mini-rocker shaker	V.4AW
MR-12, rocker-shaker	V.4AW

1.1.1. Revision number: 4.05.

1.1.2. Release date: April of 2026.

1.2. Symbols used in this IFU:



Caution! Please pay special attention to sections marked by this symbol.

2. Safety precautions

2.1. General warnings:



Caution! Make sure you have fully read and understood the present Manual before using the equipment.

2.2. Icons used on the unit and packaging:

	CE marking, manufacturer affirms conformity with European health, safety, and environmental protection standards, see 12.1
	WEEE directive marking, see 12.1
	Polarity of the power connector
	Equipment uses direct current

2.3. General safety

- The protection provided can be ineffective if the operation of the appliance does not comply with the manufacturer's requirements.
- Save the unit from shocks and falling.
- Store and transport the unit as described in section **Storage and transportation**.
- Use only original parts and accessories, provided by manufacturer for this product.
- Before using any cleaning or decontamination methods except those recommended by the manufacturer, check with the manufacturer that the proposed method will not damage the equipment.
- Do not make modifications in design of the unit.

2.4. Electrical safety

- Connect only to external power supply with voltage corresponding to that on the serial number label.
- Ensure that the external power supply and plug are easily accessible during use.
- Do not plug the unit into an ungrounded power socket, and do not use an ungrounded extension lead.
- Disconnect the unit from the mains before moving.
- If liquid penetrates into the unit, disconnect it from the mains and have it checked by a repair and maintenance technician.
- Do not operate the unit in premises where condensation can form. Operating conditions of the unit are defined in section **Specifications**.

2.5. During operation

- Do not impede the platform motion.
- Do not place objects between the platform and the unit.
- Do not operate the unit in environments with aggressive or explosive chemical mixtures. Please contact manufacturer for operation of the unit in specific atmospheres.
- Do not use outside the laboratory rooms.
- Do not operate the unit if it is faulty or has been repaired incorrectly.
- Do not place a load exceeding the maximum load value mentioned in section **Specifications**.

2.6. Biological safety

- It is the user's responsibility to carry out appropriate decontamination if hazardous material is spilt on or penetrates into the equipment.

3. General information

3.1. Model description and uses. MR-1 and MR-12 rocker-shakers are designed for mixing solutions or media in vessels or single-use plastic bags (MR-12). The platform has a non-slip, heat-resistant silicone mat for stability, with optional PDM mat for tube fixation (MR-1). They are used for gel washing after electrophoresis, blotting (Southern, Northern, Western), biomolecule hybridization, and staining or washing of strips and slides.

3.1.1. MR-1 is a compact, quiet unit for individual use with a 1 kg load, constant amplitude, and continuous operation up to 7 days.

3.1.2. MR-12 supports soft and intensive shaking, up to 5 kg load, adjustable amplitude, and is suitable for cell culture in bioreactor bags up to 5 L, including bioreactor use.

3.2. **Provided functions.** Both models provide smooth speed control, time setting and display, automatic stop, operation interruption, and platform rocking. MR-12 adds overload detection with sound signal. Operating temperature range is +4 °C to +40 °C for use in cold rooms or incubators.

4. Getting started

4.1. **Unpacking.** Remove packing materials carefully and retain them for future shipment or storage of the unit. Examine the unit carefully for any damage incurred during transit. The warranty does not cover in-transit damage. Warranty covers only the units transported in the original package.

4.2. **Complete set.** Package contents:

4.2.1. MR-1

- Mini-rocker-shaker **MR-1** 1 pce.
- Detachable platform Bio PP-4S with silicone mat 1 pce.
- External power supply 1 pce.
- Instructions for use, declaration of conformity 1 copy
- PDM Dimpled mat..... 1 pce., on request

4.2.2. MR-12


- Rocker-shaker **MR-12** 1 pce.
- Detachable platform PP-480 with silicone mat 1 pce.
- 4 screws and a hex key 1 set
- External power supply 1 pce.
- Power cable 1 pce.
- Instructions for use, declaration of conformity 1 copy



Bio PP-4S
with silicone mat



Bio PP-4S
with dimpled mat PDM

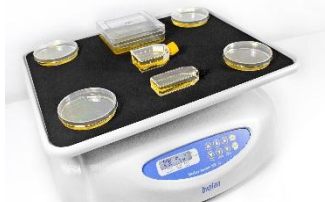

PP-480
with silicone mat

4.3. **Setup:**

- Place the unit upon firm stable even horizontal surface;
- Remove protective film from the display;
- Connect the power cord to the external power supply;
- Plug the external power supply into the 12 V socket at the rear side of the unit.

4.4. **Platform setup.**

4.4.1. Model **MR-1**. Install the platform on the moving base by fitting the pins on the platform with openings on the base.

4.4.2. Model **MR-12**. Install the platform on the unit and remove the silicone pad. Secure the platform on the supporting platform on top of the unit with the four supplied screws. Cover the platform with the silicone mat.

5. Operation – model MR-1

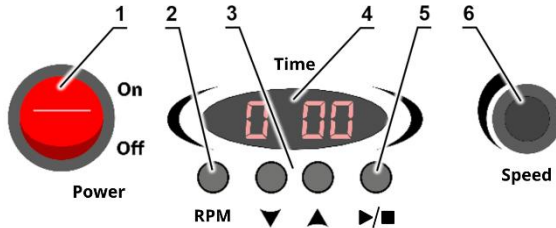


Figure 1. MR-1, control panel

5.1. Connect the external power supply to a grounded mains outlet. Switch **on** the **Power** switch (fig. 1/1). Display powers up (fig. 1/4)

5.2. Place the samples on the platform, balancing the load equally in relation to the axle.



Caution! It is forbidden to place any items between platform and body of the unit.

5.3. **Setting time.** Using **▲** and **▼** keys (fig. 1/3), set the necessary time interval in hours and minutes (step 1 minute), as shown on the display (fig. 1/4). If a key is held down for long time, values change faster.

5.4. **Setting speed.** Using the **Speed** knob (fig. 1/6), set the necessary shaking speed. When turning the knob or pressing the **RPM** key (fig. 1/2), the display (fig. 1/3) shows speed in rockings per minute (RPM).

5.5. Press the **▶/■** key (fig. 1/5). Platform begins movement and timer starts counting elapsed time, for values below 1 hour- in minutes and seconds (mm:ss), above 1 hour – in minutes (hh:mm). Speed can be changed during operation.

5.6. If the time interval is set to 0:00, then pressing the **▶/■** key puts the unit in continuous operation mode, until the **▶/■** key is pressed again.

5.7. Platform stops after the set time interval elapses.

5.8. The operation can be stopped at any time before time interval elapses by pressing the **▶/■** key. The platform reaches horizontal position and stops. Display shows elapsed time for 20 seconds, then changes back to set time interval.

5.9. To repeat the operation with the same time interval, press the **▶/■** key.

5.10. To reset the time interval, press and hold the **▶/■** key for more than 3 seconds.

5.11. After finishing the operation, switch **off** the **Power** switch and disconnect the external power supply from the mains outlet.

6. Operation – model MR-12

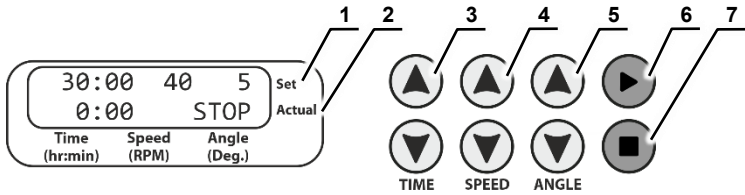


Figure 2. MR-12, control panel

- 6.1. Connect the external power supply to a grounded mains outlet.
- 6.2. Place the samples on the platform, balancing the load equally in relation to the axle.
⚠ Caution! Do not place any items between platform and body of the unit.
- 6.3. Display shows previously set time, speed and angle in the upper **Set** line (fig. 2/1), and elapsed time and mode indication in the lower **Actual** line (fig. 2/2).
- 6.4. **Setting time.** Using ▲ and ▼ **TIME** keys (fig. 2/3), set the necessary time interval in hours and minutes (step 1 minute).
- 6.5. **Setting speed.** Using ▲ and ▼ **SPEED** keys (fig. 2/4), set the necessary mixing speed in rockings per minute (step 1 RPM).
⚠ Note. If the speed is set higher than 50 RPM, then the angle is locked to 10°
- 6.6. **Setting angle.** Using ▲ and ▼ **ANGLE** keys (fig. 2/5), set the necessary angle in degrees (step 1°).
⚠ Note. If a key is held down for long time, values change faster.
- 6.7. Press the ► key (fig. 2/6). Platform begins movement and timer starts counting elapsed time. Speed and angle can be changed during operation (but not time).
- 6.8. If the time interval is set to 0:00, then pressing the ► key puts the unit in continuous operation mode, until the ■ key (fig. 2/7) is pressed.
- 6.9. Platform stops after the set time interval elapses. Display shows indication STOP and the unit sounds a repeating signal. Press the ■ key to stop the signal.
- 6.10. The operation can be stopped at any time before time interval elapses by pressing the ■ key. The platform reaches horizontal position and stops.
- 6.11. To repeat the operation with the same time interval, press the ► key.
- 6.12. To reset the time interval, press and hold the ■ key for more than 3 seconds.
- 6.13. If the platform is overloaded, the device will make three attempts to restart the operation (display indication: DRIVER ERROR). If attempts fail, flashing OVERLOAD indication shows on the display, accompanied by a repeating sound signal, until the ■ key (fig. 2/7) is pressed. Eliminate causes of overload before restarting operation.
- 6.14. After finishing the operation, disconnect the external power supply from the mains outlet.

7. Specifications

7.1. Biosan is committed to a continuous program of improvement and re-serves the right to alter design and specifications of the equipment without additional notice.

7.2. Movement specifications

	MR-1	MR-12
Mixing frequency range	5–30 RPM	1–99 RPM
Mixing frequency setting step	1 RPM	
Tilt angle	Fixed 7°	1–10° (at 1–50 RPM)
		Fixed 10° (>50 RPM)
Motor	Brushless	
Drive	Direct	Synchronised belted
Digital time setting	1 min. - 23 h 59 min. / non-stop	1 min. - 99 h 59 min. / non-stop
Digital time setting step	1 min.	
Maximum continuous operation time	168 h	

7.3. General specifications

	MR-1	MR-12
Maximum load	1 kg	5 kg
Platform working area	215×215 mm	480×380 mm
Dimensions, W×D×H	220×205×120 mm	430×480×210 mm
Operating voltage and current	12 V=, 320 mA	12 V=, 1.1 A
Power consumption	3.8 W	13 W
External power supply	in 100–240 V~, 50–60 Hz, out 12 V=	
Weight, accurate within ± 10%	2.1 kg	11.9 kg

7.4. Workroom requirements.

Workroom description	Cold rooms, incubators (except CO ₂ incubators) and closed laboratory rooms
Temperature range	+4 °C ... +40 °C
Humidity requirements	Maximum of 80% RH at 31 °C, decreasing linearly to 50% RH at 40 °C. Non-condensing atmosphere.
Operating height, maximum	2000 m ASL
Overvoltage category	I
Pollution degree	2

8. Ordering information

8.1. Models and versions available:

Model	Version	Power supply plug	Catalogue number
MR-1 , Mini-Rocker Shaker	V.4AW	Europlug (EU; types C/E/F/K)	BS-010152-AAG
		Multiplug (US, UK, AU; types B/G/I)	BS-010152-AAK
MR-12 , Rocker-Shaker	V.4AW	EU (type C/E/F/K)	BS-010130-AAI
		UK (type G)	BS-010130-AAQ
		AU (type I)	BS-010130-AA4
		US (type B)	BS-010130-AAJ

8.2. To inquire about or order the optional accessories or the replacement parts, contact Biosan or your local Biosan representative.

8.2.1. Optional accessories:

Description	Catalogue number
PDM for MR-1 , dimpled mat for securing differently sized tubes	PDM

8.2.2. Replacement parts:

Description	Catalogue number
PP-480 for MR-12 , detachable platform with heat-resistant non-slip silicon mat	BS-010130-AK
Bio PP-4S for MR-1 , detachable platform with heat-resistant non-slip silicon mat	BS-010125-AK

9. Care and maintenance

9.1. Service.

9.1.1. If the unit is disabled (e.g., no platform movement, no reaction to key presses, etc.) or requires maintenance, disconnect the unit from the mains and contact Biosan or your local Biosan representative.

9.1.2. All maintenance and repair operations (except listed below) must be performed only by qualified and specially trained personnel.

9.1.3. Operating integrity check. If the unit follows the procedure described in sections **Operation**, then no additional checks are required.

9.2. Cleaning and disinfection.

9.2.1. Use mild soap and water with a soft cloth or sponge for cleaning the exterior. Rinse remaining washing solution with distilled water. Wipe dry the excess water with clean, soft cloth or sponge.

9.2.2. To disinfect the plastic and metal parts, use 75% ethanol or DNA/RNA removing solution (e.g., Biosan PDS-250). After disinfecting, wipe the surfaces dry.

9.2.3. Platforms and mats are autoclavable, at 121°C, for 15 min, the unit itself is not autoclavable.

9.3. **Decommissioning of the unit.** The user is responsible for the decontamination of the unit before decommissioning. Dispose of the appliance as electronic equipment in accordance with the relevant national laws.

10. Storage and transportation

10.1. Store and transport the unit in a horizontal position (see package label) at ambient temperatures between -20°C and +60°C and maximum relative humidity of 80%.

10.2. After transportation or storage and before connecting it to the electric circuit, keep the unit under room temperature for 2-3 hrs.

10.3. For extended storage, the unit does not require special procedures.

11. Warranty

11.1. The Manufacturer guarantees the compliance of the unit with the requirements of Specifications, provided the Customer follows the operation, storage and transportation instructions.

11.2. The warranted service life of the unit from the date of delivery to the Customer is 24 months. For extended warranty, see **11.5**.

11.3. Warranty covers only the units transported in the original package.

11.4. If any manufacturing defects are discovered by the Customer, an unsatisfactory equipment report shall be compiled, certified and sent to the local distributor address. To obtain the claim form, visit section **Technical support** on our website at link below.

11.5. Extended warranty.

- For **MR-12**, a *Premium* class model, one year of extended warranty is available free of charge after registration, during 6 months from the date of sale. Online registration form can be found in section **Warranty registration** on our website at the link below.
- For **MR-1**, a *Basic Plus* class model, extended warranty is a paid service. Contact your local Biosan representative or our service department through the **Technical support** section on our website at the link below.

11.6. Description of the classes of our products is available in the **Product class description** section on our website at the link below.

Technical support



biosan.lv/en/support

Warranty registration



biosan.lv/register-en

Product class description



biosan.lv/classes-en

11.7. The following information will be required in the event that warranty or post-warranty service comes necessary. Complete the table below and retain for your records.

Model	Serial number	Date of sale
MR-1, MR-12 Rocker-shakers		

11.8. **Production date.** Production date is placed in the serial number, on the label of the unit. Serial number consists of 14 digits styled XXXXXYYMMZZZZ, where XXXXXX is model code, YY and MM – year and month of production, ZZZZ – unit number.

12. EU Declaration of conformity

12.1. Mini-rocker shaker **MR-1** and rocker-shaker **MR-12** are in conformity with the following relevant Union legislations:

LVD 2014/35/EU	LVS EN 61010-1:2011 + A1:2019 Safety requirements for electrical equipment for measurement, control, and laboratory use. General requirements. LVS EN 61010-2-051:2021 + A11:2021 Particular requirements for laboratory equipment for mixing and stirring.
EMC 2014/30/EU	LVS EN 61326-1:2013 Electrical equipment for measurement, control and laboratory use. EMC requirements. General requirements.
RoHS3 2015/863/EU	Directive on the restriction of the use of certain hazardous substances in electrical and electronic equipment.
WEEE 2012/19/EU	Directive on waste electrical and electronic equipment.

12.2. Declaration of Conformity is available for download on the page for the relevant model on our website by links below, in the **Downloads** section:



[MR-1](#)



[MR-12](#)



Biosan SIA

Ratsupites 7 k-2, Riga, LV-1067, Latvia

Phone: +371 67426137

<https://biosan.lv/>

Edition 4.05 – April of 2026